

User's Manual

Model ISC40G(S)

Sensors and Fittings for Inductive
Conductivity Measurement



(BG)

Всички улътвания за продукти от серията ATEX Ex се предлагат на английски език. Ако се нуждаете от улътвания за продукти от серията Ex на родния ви език, се свържете с най-близкия офис или представителство на фирма Yokogawa.

(CZ)

Všechny uživatelské příručky pro výrobky, na něž se vztahuje nevýbušné schválení ATEX Ex, jsou dostupné v angličtině. Požadujete-li pokyny týkající se výrobků s nevýbušným schválením ve vašem lokálním jazyku, kontaktujte prosím vaši nejbližší reprezentační kancelář Yokogawa.

(D)

Alle Betriebsanleitungen für ATEX Ex bezogene Produkte stehen in den Sprachen Englisch. Sollten Sie die Betriebs- anleitungen für Ex-Produkte in Ihrer Landessprache benötigen, setzen Sie sich bitte mit Ihrem örtlichen Yokogawa-Vertreter in Verbindung.

(DK)

Alle brugervejledninger for produkter relateret til CE er tilgængelige på engelsk. Skulle De ønske yderligere oplysninger om håndtering af CE produkter på eget sprog, kan De rette henvendelse herom til den nærmeste Yokogawa afdeling eller forhandler.

(EST)

Kõik ATEX Ex toodete kasutamisjuhendid on esitatud inglise keeles. Ex seadmete muuakeelse dokumentatsiooni saamiseks pöörduge lähiima lokagava (Yokogawa) kontori või esindaja poole.

(E)

Todos los manuales de instrucciones para los productos antiexplosivos de ATEX están disponibles en inglés. Si desea solicitar las instrucciones de estos artículos antiexplosivos en su idioma local, deberá ponerse en contacto con la oficina o el representante de Yokogawa más cercano.

(F)

Tous les manuels d'instruction des produits ATEX Ex sont disponibles en langue anglaise. Si vous nécessitez des instructions relatives aux produits Ex dans votre langue, veuillez bien contacter votre représentant Yokogawa le plus proche.

(GB)

All instruction manuals for ATEX Ex related products are available in English. Should you require Ex related instructions in your local language, you are to contact your nearest Yokogawa office or representative.

(GR)

Ολα τα εγχειρίδια λειτουργίας των προϊοντων με ATEX Ex διατίθενται στα Αγγλικά. Σε περιπτώση πων χρειαζεστε οδηγιες σχετικα με Ex στην τοπική γλώσσα παρακαλούμε επικοινωνηστε με το πλησιεστερο γραφειο της Yokogawa η αντιπροσωπο της.

(H)

Az ATEX Ex műszerek gépkönyveit angol nyelven adjuk ki. Amennyiben helyi nyelven kérík az Ex eszközök leírásait, kérjük keressék fel a legközelebbi Yokogawa irodát, vagy képviseletet.

(I)

Tutti i manuali operativi di prodotti ATEX contrassegnati con Ex sono disponibili in inglese. Se si desidera ricevere i manuali operativi di prodotti Ex in lingua locale, mettersi in contatto con l'ufficio Yokogawa più vicino o con un rappresentante.

(LV)

Visas ATEX Ex kategorijas izstrādājumu Lietoðanas instrukcijas tiek piegādātas angīu valodās. Ja vçlaties saðemt Ex ierīeu dokumentāciju citā valodā, Jums ir jåsazinās ar firmas Yokogava (Yokogawa) tuvāko ofisu vai pârstāvi.

(LT)

Visos gaminiø ATEX Ex kategorijos Eksplotavimo instrukcijos teikiami anglø kalbomis. Nor dami gauti priestaisø Ex dokumentacij  kitomis kalbomis susisiekite su artimiausiu bendrov s Yokogawa biuru arba atstovu.

(M)

Il-manwali kollha ta' l-istruzzjonijiet ghal prodotti marbuta ma' ATEX Ex huma disponibbli bl-Ingl z. Jekk tkun tehtie  struzzjonijiet marbuta ma' Ex fil-lingwa lokali tieghek, ghandek tikkuntattja lill-eqreb rappre zentan jew uffic ju ta' Yokogawa.

(NL)

Alle handleidingen voor producten die te maken hebben met ATEX explosiebeveiliging (Ex) zijn verkrijgbaar in het Engels. Neem, indien u aanwijzingen op het gebied van explosiebeveiliging nodig hebt in uw eigen taal, contact op met de dichtstbijzijnde vestiging van Yokogawa of met een vertegenwoordiger.

(P)

Todos os manuals de instru es referentes aos produtos Ex da ATEX est o dispon veis em Ingl s. Se necessitar de instru es na sua l ngua relacionadas com produtos Ex, dever  entrar em contacto com a delega o mais pr xima ou com um representante da Yokogawa.

(PL)

Wszystkie instrukcje obslugi dla urz dze  w wykonaniu przeciwwybuchowym Ex, zgodnych z wymaganiami ATEX, dost pne s  w j zyku angielskim. Je eli wymagana jest instrukcja obslugi w Pa stwa lokalnym j zyku, prosimy o kontakt z najbli szym biurem Yokogawy.

(RO)

Toate manualele de instructiuni pentru produsele ATEX Ex sunt in limba engleza. In cazul in care doriti instructiunile in limba locala, trebuie sa contactati cel mai apropiat birou sau reprezentant Yokogawa.

(S)

Alla instruktionsb cker f r ATEX Ex (explosionss kra) produkter  r tillg ngliga p  engelska. Om Ni beh ver instruktioner f r dessa explosionss kra produkter p  annat spr k, skall Ni kontakta n rmaste Yokogawakontor eller representant.

(SF)

Kaikkien ATEX Ex-typpisten tuotteiden kyttoh jeet ovat saatavilla englannin-. Mik li tarvitsette Ex-typpisten tuotteiden ohjeita omalla paikallisella kieell nnne, ottakaa yhteytt  l himp n Yokogawa-toimistoon tai -edustajaan.

(SK)

V setky n vody na obsluhu pre pr stroje s ATEX Ex s  k dispoz ci i v jazyku anglickom. V pr pade potreby n vodu pre Ex-pr stroje vo Va om n rodnom jazyku, skontaktujte prosim miestnu kancel riu firmy Yokogawa.

(SLO)

Vsi predpisi in navodila za AEX Ex sorodni pridelki so pri roki v angleščini. Èe so Ex sorodna navodila potrebna v va em tukejnjem jeziku, kontaktirajte va  najbli hi Yokogawa office ili predstaunka.

Table of Contents

| | |
|--|-----------|
| 1 INTRODUCTION | 7 |
| 1.1 General | 7 |
| 1.2 Unpacking and Checking | 7 |
| 1.3 Warranty and Service | 7 |
| 1.4 Serial Number definition | 8 |
| 2 GENERAL SPECIFICATIONS | 9 |
| 2.1 Measuring elements | 9 |
| 2.2 Materials | 9 |
| 2.3 Functional specifications (at 25°C) | 9 |
| 2.4 Dynamic specifications | 9 |
| 2.5 Operating range | 10 |
| 2.6 Regulatory standards | 10 |
| 2.7 Shipping details | 11 |
| 2.8 Environmental conditions | 11 |
| 2.9 Process connections | 11 |
| 3 INSTALLATION OF SENSOR WITH STANDARD OPTIONS | 14 |
| 3.1 Typical installation | 14 |
| 3.1.1 Installation of ISC40G(S)-GG (TG) with flange adapters | 14 |
| 3.1.2 Installation of ISC40G(S)-TG with T-piece | 16 |
| 3.1.3 Installation of ISC40G(S)-GS with flange adapters | 17 |
| 4 DIMENSIONS ISC40 SENSOR | 18 |
| 5 WIRING ISC40 SENSOR | 19 |
| 6 MODELCODE ISC40 SENSOR | 20 |
| 7 SPAREPARTS ISC40 SENSOR | 21 |
| 8 EU DECLARATION OF CONFORMITY | 22 |
| 9 ISC40FS – FLOW FITTING SUBASSEMBLY | 23 |
| 9.1 General Specifications | 23 |
| 9.1.1 Materials | 23 |
| 9.1.2 Operating range | 23 |
| 9.1.3 Shipping details | 23 |
| 9.1.4 Process connections | 23 |
| 9.2 Installation of ISC40 sensor in ISC40FS | 23 |
| 9.3 Dimensions ISC40FS | 24 |
| 9.4 Modelcode ISC40FS | 25 |
| 9.5 Spareparts ISC40FS | 25 |

| | |
|--|-----------|
| 10 ISC40FF – FLOW FITTING | 26 |
| 10.1 General Specifications | 26 |
| 10.1.1 Materials | 26 |
| 10.1.2 Operating range | 26 |
| 10.1.3 Shipping details | 26 |
| 10.1.4 Process connections | 26 |
| 10.2 Installation of ISC40 sensor in ISC40FF | 26 |
| 10.3 Dimensions ISC40FF | 27 |
| 10.4 Modelcode ISC40FF | 28 |
| 10.5 Spareparts ISC40FF | 29 |
| 11 ISC40FD – IMMERSION FITTING | 30 |
| 11.1 General Specifications | 30 |
| 11.1.1 Materials | 30 |
| 11.1.2 Operating range | 30 |
| 11.1.3 Process connections | 30 |
| 11.2 Installation of ISC40 sensor in ISC40FD | 30 |
| 11.3 Dimensions ISC40FD | 32 |
| 11.4 Modelcode ISC40FD | 33 |
| 11.5 Spareparts ISC40FD | 33 |
| 12 Chemical Compatibility Chart | 34 |

1 INTRODUCTION

1.1 General

The sensor and fitting program for inductive conductivity measurement (model ISC40) is designed to meet the most common installation requirements in terms of material compatibility, process connections and flow dynamics. The various installation possibilities are described and illustrated in this manual.

The following categories of installation can be recognised:

1. Direct mounting of sensors in tank wall or customer supplied flanges
2. Cost effective installation of sensors using process adapters
3. Maintenance friendly installation of sensors using in-line subassemblies
4. Installation in flow chambers for measurements in sample streams or bypass loops
5. Installation in immersion fittings for measurement in open tanks or channels

Within the wide range of process adapters, subassemblies, flow fittings and immersion fittings it is easy to find the appropriate installation that fits the application (a wide choice of materials), the plant installation practice (a wide choice of process connections) and the maintenance procedures.

1.2 Unpacking and Checking

Upon delivery, unpack the sensor carefully and inspect it to ensure that it is not damaged during shipment. If damage is found, retain the original packing material and immediately notify the carrier and the relevant local Yokogawa Sales office. Make sure the Model Code and Serial Number on the sensor are the same as on the packing list. Also check if option(s) that were ordered, are included and correct.

1.3 Warranty and Service

Yokogawa products are guaranteed free from defects in workmanship and materials under normal use and service for a period of (typically) 12 months from the date of shipment from the manufacturer. Individual Sales organizations can deviate from the typical warranty period, and the conditions of sale relating to the original purchase order should be consulted. Damage caused by wear and tear, inadequate maintenance, corrosion, or by the effects of chemical processes is excluded from this warranty coverage. In the event of a warranty claim, the defective goods should be sent (freight paid) to the Service Department of the relevant Yokogawa Sales office for repair or replacement (at Yokogawa's discretion).

The following information must be included in the letter accompanying the returned goods:

- Model Code and Serial Number.
- Original Purchase Order and Date.
- Length of time in service and description of the process.
- Description of the fault and circumstances of the failure.
- Process/environmental conditions that may be related to the failure of the sensor.
- Statement as to whether warranty or non-warranty service is requested.
- Complete shipping and billing instructions for return of material, plus the name and phone number of a contact person that can be reached for further information.
- Clean Statement

Returned goods that have been in contact with process fluids must be decontaminated and disinfected prior to shipment. Goods should carry a certificate to this effect, for the health and safety of our employees. Material Safety Data sheets must be included for all components of the process to which the sensor(options) have been exposed.

1.4 Serial Number definition

The Serial Number is defined by nine (9) alphanumeric characters:

| | |
|--|---------------------|
| X ₁ X ₂ | Production Location |
| X ₃ X ₄ | Year/Month code |
| X ₅ X ₆ X ₇ X ₈ X ₉ | Tracking number |

Example: N3P600028

Method used for year/month numbering

Table 1: Production Year code

| Year | Year code | Year | Year code |
|-------------|------------------|-------------|------------------|
| 2014 | P | 2026 | 3 |
| 2015 | R | 2027 | 4 |
| 2016 | S | 2028 | 5 |
| 2017 | T | 2029 | 6 |
| 2018 | U | 2030 | 7 |
| 2019 | V | 2031 | 8 |
| 2020 | W | 2032 | 9 |
| 2021 | X | 2033 | A |
| 2022 | Y | 2034 | B |
| 2023 | Z | 2035 | C |
| 2024 | 1 | 2036 | D |
| 2025 | 2 | 2037 | E |

Table 2: Production Month code

| Month | Month code |
|--------------|-------------------|
| January | 1 |
| February | 2 |
| March | 3 |
| April | 4 |
| May | 5 |
| June | 6 |
| July | 7 |
| August | 8 |
| September | 9 |
| October | A |
| November | B |
| December | C |

2 GENERAL SPECIFICATIONS

The ISC40 inductive conductivity sensor is suitable for use with the Yokogawa inductive conductivity analyzers.

2.1 Measuring elements

: Toroids with high permeability magnetic material
Pt1000 or 30k temperature element

2.2 Materials

Wetted parts sensor

Body ISC40*-G* : 30% glass filled PEEK, FDA approved
Body ISC40*-T* : PFA, FDA approved, PIM regulation 10/2011 approved

Non-wetted parts sensor

Sealing gasket : Viton
Thread part : AISI 316 SS

Options for sensor

All options except /TFD: AISI 316 SS and O-ring material as wetted part
/TFD : AISI 316 SS as non-wetted part
TFM and Kalrez as wetted part

2.3 Functional specifications (at 25°C)

Temperature element : Pt1000 to IEC 751
30k NTC
Installation factor : 1.88 cm⁻¹ nominal for PEEK sensor
3.00 cm⁻¹ nominal for PFA sensor
Actual installation can change this factor.
If there is less than 25mm spacing between sensor and holder,
in-situ calibration is necessary to meet the specified accuracies
(see fig. 1)

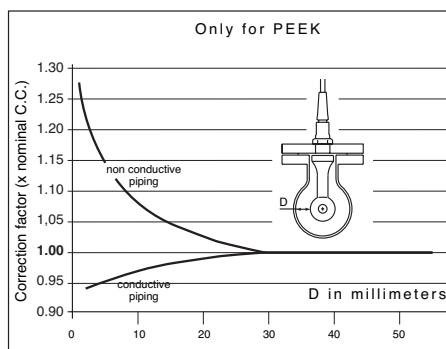


Fig 1: Actual installation factor as function of spacing around the sensor

Note: The ISC40 temperature sensor is designed for cell compensation and for indication.
It is **NOT** designed for process temperature control.

2.4 Dynamic specifications

Response time : $t_{90} < 5$ min. for PEEK sensor
conductivity $t_{90} < 10$ min. for PFA sensor

2.5 Operating range

Conductivity : 0 – 2000 mS/cm at actual process temperature.

Note: The sensor has an error (0.5 µS/cm for PEEK model, 1.0 µS/cm for PFA model) that must be considered when application is chosen.

| | |
|--------------|--|
| Temperature | : -20°C to 130°C (-4°F to 266°F) |
| Pressure | : 0 to 20 bar (0 to 290 PSIG) for PEEK sensor 0 to 15 bar (0 to 217 PSIG) for PFA sensor. |
| Cable length | : max 50 meter, in combination with WF10 extension cable and BA10 junction box |

2.6 Regulatory standards

CE : Decision 768/2008/EC

- ATEX : Directive 94/9/EC, as amended by Regulation (EC) no. 1882/2003

Certificate no. : DEKRA 11ATEX0063 X
 II 1 G Ex ia IIC T4...T6 Ga

Electrical data : Sensor output circuits (permanently connected cable) connected to a certified intrinsically safe circuit with the following maximum values: $Ui = 19.1\text{ V}$; $li = 170\text{ mA}$; $Pi = 0.8\text{ W}$; $Ci = 0\text{ nF}$; $Li = 0\text{ mH}$ or certified intrinsically safe Yokogawa Inductive Conductivity transmitter model FLXA21 series, model ISC202S series or model IC200S series

Note: The effective internal capacitance Ci and the effective internal inductance Li of the sensor are depending only upon the properties and the length of the connected cable.

Special conditions (X) : T6 for Tamb. -30°C to 40°C

T5 for Tamb. -30°C to 95°C

T4 for Tamb. -30°C to 130°C, depending on sensor body material

WARNING : The sensor must be installed and used so, that dangers of ignition due to hazardous electrostatic charges cannot occur, especially in the case that the process medium is non-conductive.

- Pressure : Directive 97/23/EC, as amended by Regulation (EC) no. 1882/2003

Applying article : 3.3 (Sound Engineering Practice)

IECEx

Applying standards : IEC 60079-0 : 2007
IEC 60079-11 : 2006

IEC 60079-26: 2006

Certificate no. : IECEx DEK 11.0028X
Ex ia IIC T4...T6 Ga

CSA

| | |
|---------------------------|--|
| Certificate no. | : 2447837 IS, Class I Div. 1, GP A, B, C, D T4...T6 Master Contract no 182892 |
| Electrical data | : Sensor output circuits (permanently connected cable) connected to a certified intrinsically safe circuit with the following maximum values: Uo = 19.1 V; Io = 170 mA; Po = 0.8 W; Co ≥ Ci + Ccable; Lo ≥ Li + Lcable or certified intrinsically safe Yokogawa Inductive Conductivity transmitter model FLXA21 series, model ISC20S series or model IC200S series |
| Ambient temperature range | : T6 for Tamb. -30°C to 40°C T5 for Tamb. -30°C to 95°C T4 for Tamb. -30°C to 130°C, depending on sensor body material |

Note: Intrinsically safe when connected as per Control Drawing FF1-K1244QY (see fig. 2)

FM

| | |
|---------------------------|--|
| Certificate no. | : 3046320 IS, Class I, Div. 1, Groups A, B, C, D T4...T6 |
| Electrical data | : Sensor output circuits (permanently connected cable) connected to a FM approved intrinsically safe apparatus meeting the entity parameters of the ISC40S: Uo ≤ 19.1 V; Io ≤ 170 mA; Po ≤ 0.8 W; Co ≥ Ci + Ccable; Lo ≥ Li + Lcable or certified intrinsically safe Yokogawa Inductive Conductivity transmitter model FLXA21 series, model ISC20S series or model IC200S series |
| Ambient temperature range | : T6 for Tamb. -30°C to 40°C T5 for Tamb. -30°C to 85°C T4 for Tamb. -30°C to 85°C, depending on sensor body material |

Note: Intrinsically safe when connected as per Control Drawing FF1-K1244QX (see fig. 3)

2.7 Shipping details

| | |
|------------------------|--|
| ISC40*-**-*03 (05) | Package size (LxWxH) : 350 x 270 x 50 mm (13.8 x10.6 x 2.0 inch) |
| ISC40*-**-*10 (15, 20) | : 320 x 240 x110 mm (12.6 x 9.5 x 4.3 inch) Package weight (app.) |
| ISC40*-**-*03 | : 1.0 kg (2.2 lbs) |
| ISC40*-**-*05 | : 1.3 kg (2.9 lbs) |
| ISC40*-**-*10 | : 1.6 kg (3.5 lbs) |
| ISC40*-**-*15 | : 2.1 kg (4.6 lbs) |
| ISC40*-**-*20 | : 2.5 kg (5.5 lbs) |

2.8 Environmental conditions

| | |
|---------------------|---|
| Storage temperature | : -30°C to 50°C (-22°F to 122°F) |
| Water proof | : IP67 (conform IEC 60529), also in combination with the preferred Yokogawa process connections |

2.9 Process connections

Process connections are made in combination with a variety of adapters and fittings, which are available in AISI 316 SS, PVC or PVDF (see relevant sections in this manual).

Control Drawing CSA

The ISC40S sensor shall be installed with one of the Yokogawa transmitters model:

- ISC202S • IC200S • FLXA21

with following parameters:

| | ISC202S | IC200S | FLXA21 |
|----|----------------|---------------|---------------|
| Uo | 14.4 V | 19.1 V | 11.76 V |
| Io | 88 mA | 162 mA | 60.6 mA |
| Po | 317 mW | | 178 mW |
| Lo | 4.5 mH | 800µH | 8 mH |
| Co | 600 nF | 254nF | 100 nF |

or

To a CSA approved intrinsically safe apparatus meeting the entity parameters of the ISC40S: $U_o \leq 19.1V$

$$I_o \leq 170mA$$


$$P_o \leq 0.8W$$

$$C_o \geq C_i + C(\text{cable})$$

$$L_o \geq L_i + L(\text{cable})$$


The effective inductive capacitance C_i and the effective induced inductance L_i of the sensor depends only upon the properties and the length of the connected cable (max 50m).

When installing this equipment, follow the manufacturer's control drawing. Installing should be in accordance with Canadian Electrical Code Part 1 or CEC Part1.

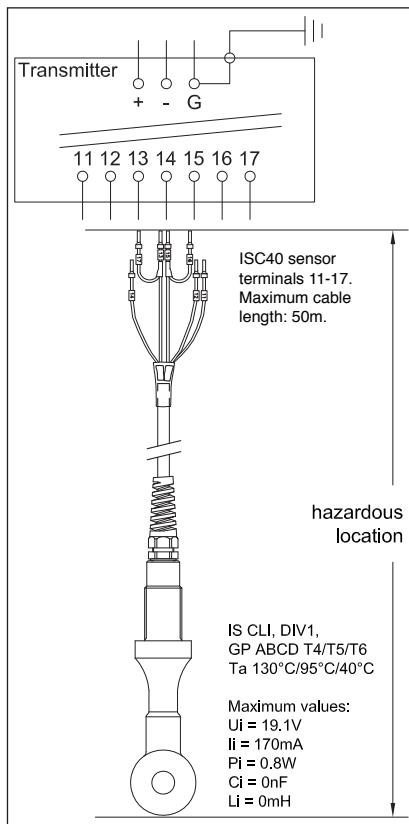

**Fig 2: FF1-K1244QY
Control Drawing CSA**

Warning: To prevent ignition of flammable or combustible atmospheres, disconnect power before servicing or read, understand and adhere to the manufacturer's live maintenance procedures.

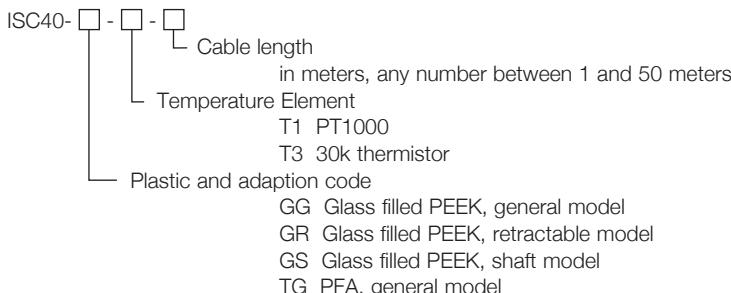

Control Drawing FM

The ISC40S sensor shall be installed with one of the Yokogawa transmitters model:

- ISC202S • IC200S • FLXA21

with following parameters:

| | ISC202S | IC200S | FLXA21 |
|----|----------------|---------------|---------------|
| Uo | 14.4 V | 19.1 V | 11.76 V |
| Io | 88 mA | 162 mA | 60.6 mA |
| Po | 317 mW | | 178 mW |
| Lo | 4.5 mH | 800 μ H | 8 mH |
| Co | 600 nF | 254nF | 100 nF |

or

To a FM approved intrinsically safe apparatus meeting the entity parameters of the ISC40S: Uo \leq 19.1V

$$Io \leq 170mA$$

$$Po \leq 0.8W$$



$$Co \geq Ci + C(\text{cable})$$

$$Lo \geq Li + L(\text{cable})$$

The effective inductive capacitance Ci and the effective induced inductance Li of the sensor depends only upon the properties and the length of the connected cable (max 50m).

When installing this equipment, follow the manufacturer's control drawing. Installing should be in accordance with ANSI/ISA RP 12.06.01 "Installation of Intrinsically Safe Systems for Hazardous (Classified) Locations" and the National Electrical Code (ANSI/NFPA 70).

Warning: To prevent ignition of flammable or combustible atmospheres, disconnect power before servicing or read, understand and adhere to the manufacturer's live maintenance procedures.

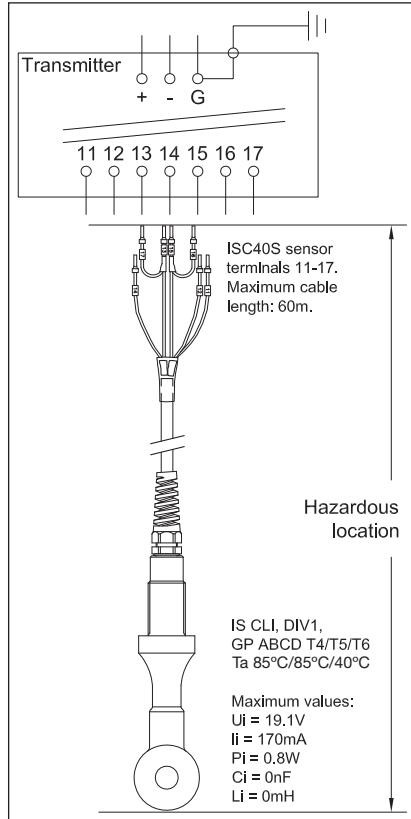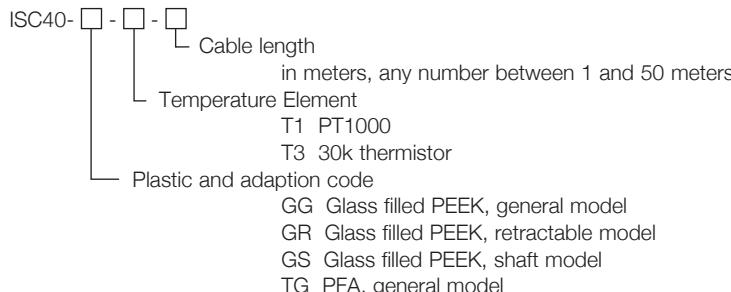

**Fig 3: FF1-K1244QX
Control Drawing FM**

3 INSTALLATION OF SENSOR WITH STANDARD OPTIONS

For optimum measurement results, the ISC40 sensor should be installed in a location that offers an acceptable representation of the process composition and **DOES NOT** exceed the specifications of the sensor.

It is important that the process flow is directed through the hole in the donut of the sensor. For this reason the flats on the sensor top part have to be installed perpendicular on the process flow (see fig. 4).

The inductive conductivity measurement technique requires a process fluid surrounding the donut of the sensor. The installation factor mentioned on the label of the sensor cable will assure accurate conductivity measurement under the condition that the donut is surrounded by 25 mm (1") process fluid. If this condition cannot be met, the measurement loop (analyser in combination with sensor) has to be calibrated. Consult the instruction manuals of the analyser for details.

The mounting of the sensor in the process adapters is described in section 3.1. The mounting of the process adapters in the end-users application requires compatibility of materials and process connections.

3.1 Typical installation

3.1.1 Installation of ISC40G(S)-GG (TG) with flange adapters

The ISC40G(S)-GG (TG) sensor is supplied with a flat Viton sealing gasket for compatibility with existing installations. When using the sensor in combination with the new fittings, which are improved by the addition of O-ring seals (see figure 6), the flat Viton gasket should be discarded.

It is important that the access port has a diameter of at least 50 mm (2") to allow insertion of the donut shaped end of the sensor. For more detailed dimensions of the sensor see paragraph 4.

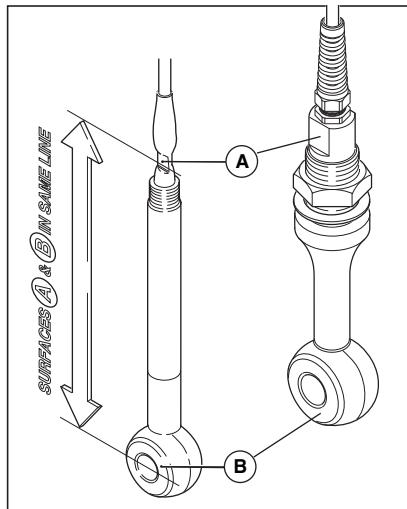


Fig 4: Aligning of sensor donut (B) and flats (A)

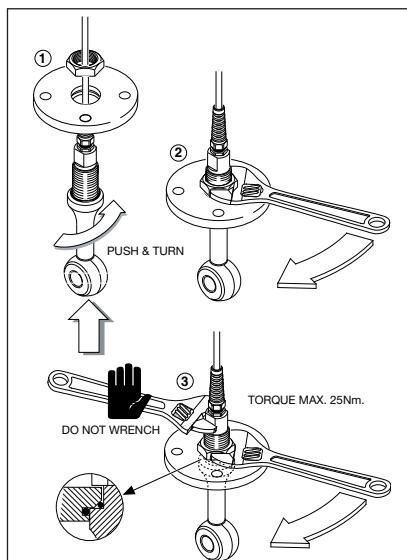


Fig 5: Mounting Procedure ISC40G(S)-GG (TG) with flange adapters

Note: When a torque of more than 25 Nm is applied, the top part of the body of the PFA sensor will be damaged (TG model)

Note: Retighten after 24 hours

The sensor cable and mounting thread are pulled through the hole of the flange, and the sensor is sealed from the process by tightening the mounting nut. Turning of the sensor by the torque forces can be

avoided by using a wrench on the flats on top of the sensor (see fig. 5). Sensor is installed correctly if the flats are aligned perpendicular on the process flow.

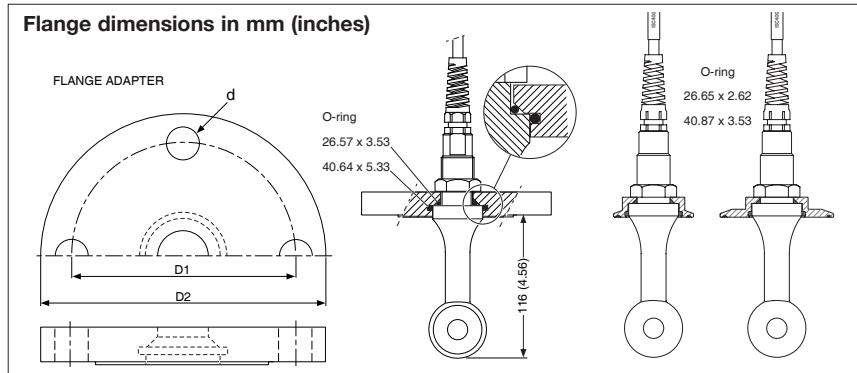


Fig 6: Option /SFA, /SFD,

/S2W, /STW

| Option | d | D1 | D2 |
|--------|------------|------------|-----------|
| /SFA | Ø19 (0.75) | 121 (4.76) | 152 (6.0) |
| /SFD | Ø18 (0.71) | 125 (4.92) | 165 (6.5) |
| /TFD | Ø18 (0.71) | 145 (5.71) | 185 (7.3) |


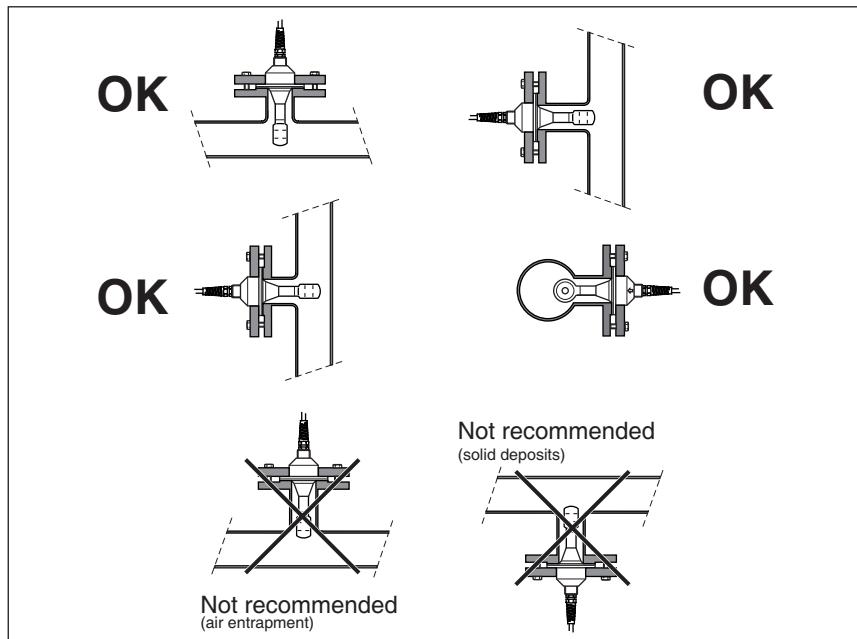


Fig 7: Installation examples

3.1.2 Installation of ISC40G(S)-TG with T-piece

The ISC40G(S)-TG sensor is a PFA sensor which can be used in combination with a T-piece of which the inner side is lined with PFA. This can be done using option /TFD (sealing material with stainless steel DN65 PN10 flange), or by option /TFN (sealing material) if the stainless steel flange DN65 PN10 is already available. Both options are available as spare part.

Note: If sensor is replaced, you have to use new sealing materials (part no. K1541XG) to prevent process leakage.

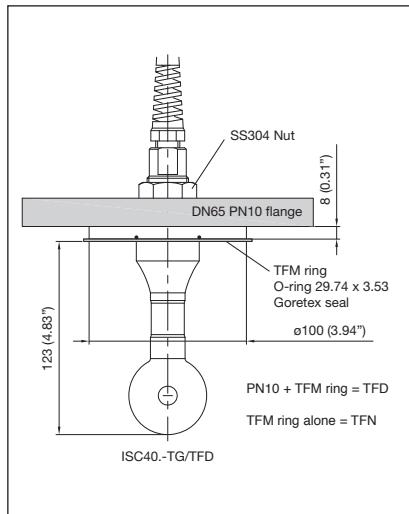

**Fig 8: Flange adapters
(option /TFD, /TFN) for -TG sensor
in combination with T-piece**

T-piece:

| Partno. | Flanges | Description |
|---------|------------|-----------------------|
| K1500HG | DN80 PN10 | T-piece, DN80 flange |
| K1500HF | DN100 PN10 | T-piece, DN100 flange |

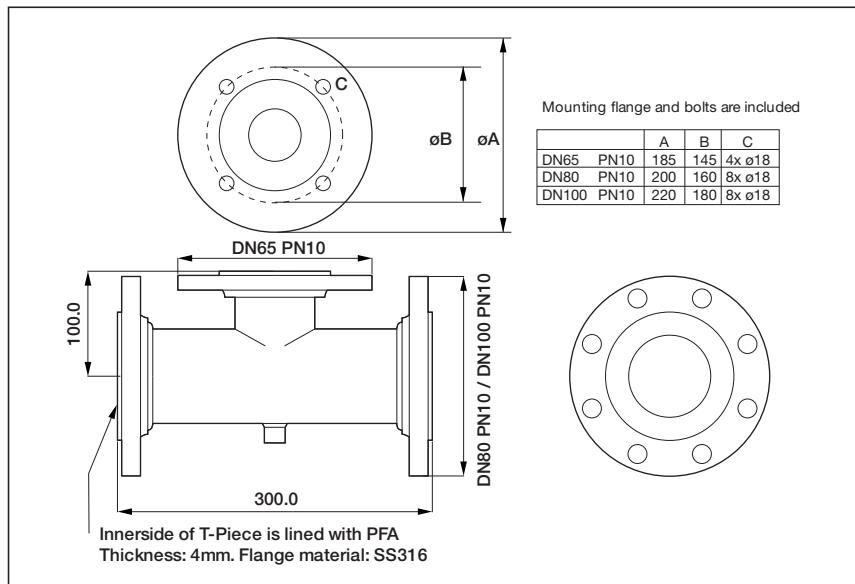


Fig 9: T-piece dimensions

3.1.3 Installation of ISC40G(S)-GS with flange adapters

The ISC40G(S)-GS sensor is designed for sanitary applications. For these applications special process connections are necessary.

Mounting procedure:

- Screw the tube completely in the stainless steel nut.
- Thread the sensor cable through the flange adapter parts in the right sequence.
- Screw the tube hand tight into the flange, a mechanical stop will be felt.
- Tighten the plastic nut onto the sensor; screw the plastic nut completely tight.
- Tighten the stainless steel nut for locking the sensor.

Sensor is installed correctly if the flats on the sensor are aligned perpendicular on the process flow.

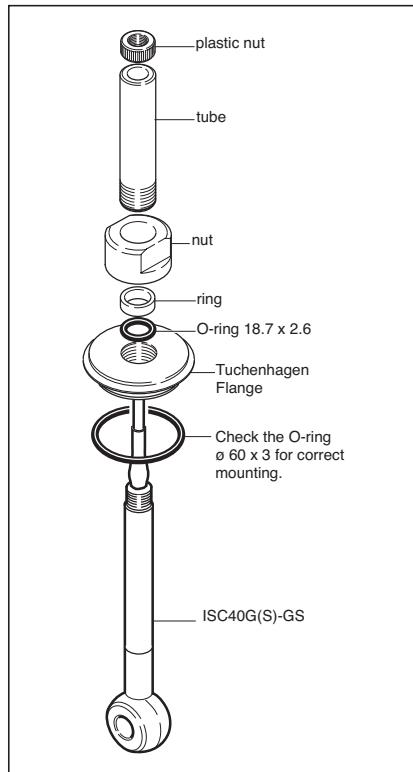


Fig 10: Installation /SFT

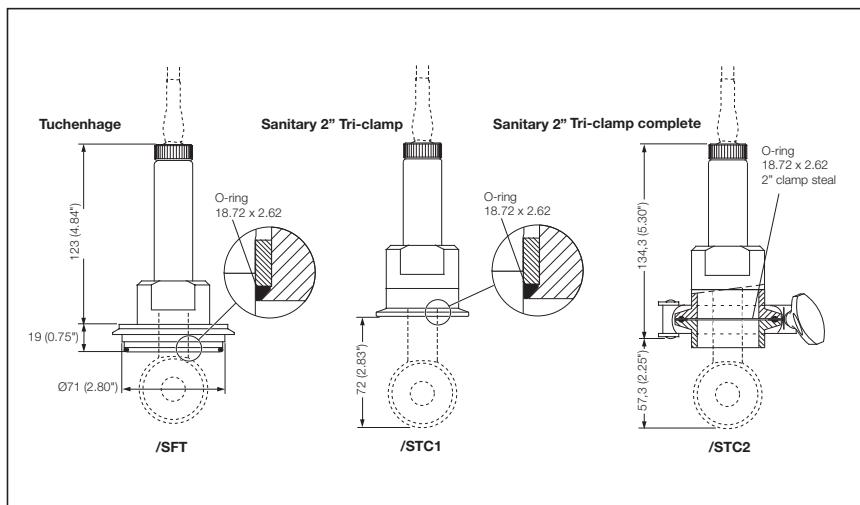


Fig 11: Option /SFT, /STC1, /STC2

4 DIMENSIONS ISC40 SENSOR

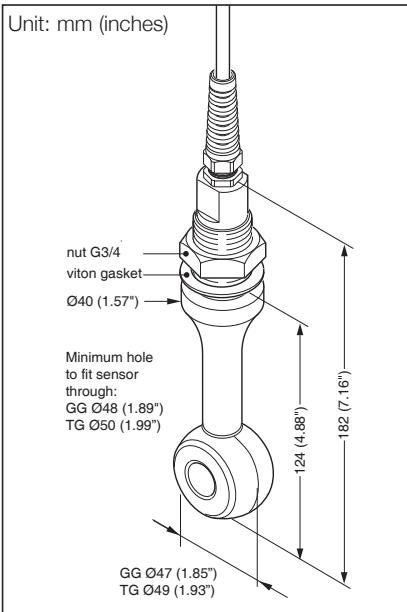


Fig 12: ISC40G(S)-GG (TG)

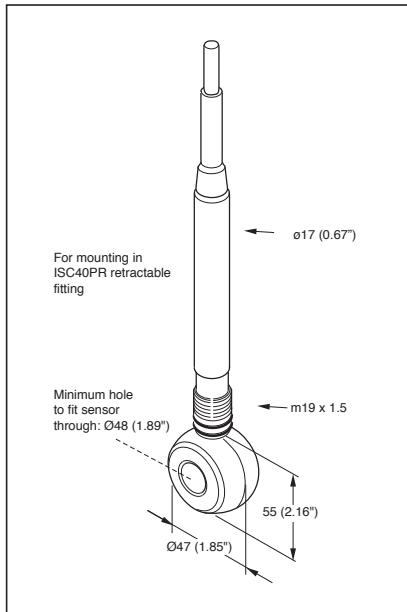


Fig 13: ISC40G(S)-GR

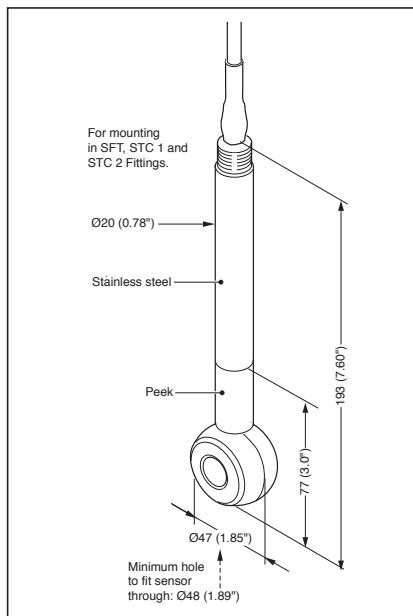



Fig 14: ISC40G(S)-GS

5 WIRING ISC40 SENSOR

The ISC40 sensor is provided with a fixed cable. The connections of this dual coax cable and the Yokogawa Inductive Conductivity analyser are given in table 1.

Table 1: Definition cable and analyzer

| Cable wire color | ISC analyser terminal # | Signal description |
|------------------|-------------------------|--------------------|
| Red | 11 | Temperature |
| Blue | 12 | Temperature |
| Yellow | 14 | Shield |
| White | 15 | Primary coil |
| White (shield) | 16 | Primary coil |
| Brown | 13 | Secondary coil |
| Brown (shield) | 17 | Secondary coil |

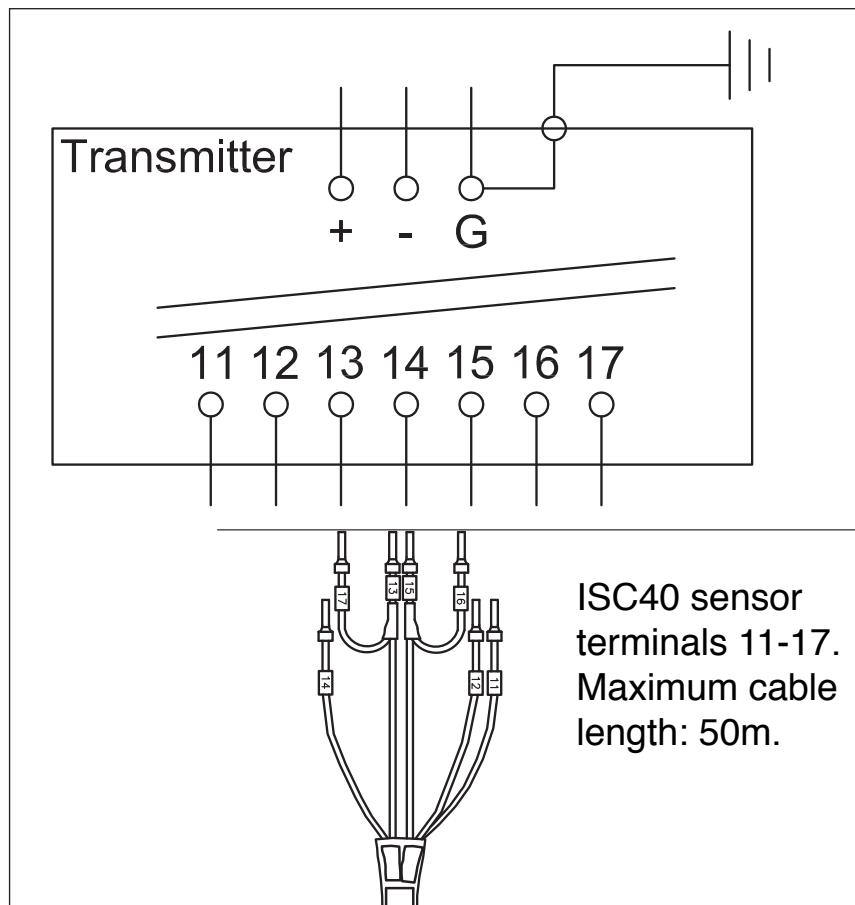

6 MODEL CODE ISC40 SENSOR

| Model Code | Suffix | Option | Description |
|----------------------------------|-------------------------------|------------------|--|
| ISC40G | | | General purpose inductive conductivity sensor |
| Sensor type | -GG | | Glass filled PEEK, general model |
| | -GR | | Glass filled PEEK, retractable model |
| | -GS | | Glass filled PEEK, shaft model |
| | -TG | | PFA, general model |
| Temperature sensor | T1 | | Pt1000 |
| | T3 | | 30k thermistor, for IC200 select only T3 |
| Cable length | -3 -5 -10 -15 -20 | | 03 meter 05 meter 10 meter 15 meter 20 meter |
| Options for Sensor | | Material | Proc. Connection |
| Flange adapters -GG, -TG | | AISI 316 SS | 2" ANSI 150 lbs |
| /SFA | | AISI 316 SS | NW50 |
| /SFD | | AISI 316 SS | 3" tri-clamp |
| /STW | | AISI 316 SS | 2" tri-clamp |
| /S2W | | AISI 316 SS | NW65-PN10 |
| /TFD | | TFM, AISI 316 SS | For NW65-PN10 |
| /TFN | | TFM | |
| Flange adapters for -GS | | AISI 316 SS | Sanitary Tuchenhagen |
| /SFT | | AISI 316 SS | Sanitary 2" tri clamp |
| /STC1 | | AISI 316 SS | Tri-clamp complete |
| /STC2 | | | |
| Protection Hose for-TF, -TG, -GG | | /PH□□ | 03m /05m /10m /15m /20m Same length as the cable |
| Certificates | | /M | Material certificate |
| | | /Q | Quality certificate Only for flange adapters except /TFD and /TFN |

7 SPAREPARTS ISC40 SENSOR

| Parts ISC40 sensor | | | | |
|--|-----------------------|--------------------|----------|-----------|
| Part no. | Description | Material | Quantity | |
| K1500AM | Gasket | Viton | 5 | |
| K1500AL | Mounting nut | AISI 316 SS | 3 | |
| Options ISC40 sensor, Flange adapters | | | | |
| Part no. | Description | Process connection | Material | O-ring(s) |
| K1541ZR /SFA | 2" ANSI 150 lbs | AISI 316 SS | Viton | |
| K1541ZQ /SFD | NW50 | AISI 316 SS | Viton | |
| K1541KB /STW | 3" tri-clamp | AISI 316 SS | EPDM | |
| K1541KC /S2W | 2" tri-clamp | AISI 316 SS | EPDM | |
| K1541XF /TFD | DN65 PN10 | AISI 316 SS, TFM | Kalrez | |
| K1541XG /TFN | used with DN65 PN10 | TFM | Kalrez | |
| K1541ZP /SFT | Sanitary Tuchenhagen | AISI 316 SS | EPDM | |
| K1541ZG /STC1 | Sanitary 2" tri-clamp | AISI 316 SS | EPDM | |
| K1541ZF /STC2 | Tri-clamp complete | AISI 316 SS | EPDM | |
| K1500HG | T-piece, DN80 flange | DN80 PN10 | | |
| K1500HF | T-piece, DN100 flange | DN100 PN10 | | |

Note: Other O-ring materials are available as sparepart

| O-rings ISC40 sensor, Flange adapters | | | | |
|--|-------------|---|----------|----------|
| Part no. | Description | Dimensions | Material | Quantity |
| O-rings /SFA, /SFD | | | | |
| K1500CA | O-ring set | 40.64 x 5.33; 26.57 x 3.53 | EPDM | 5 sets |
| K1500CB | O-ring set | 40.64 x 5.33; 26.57 x 3.53 | Viton | 5 sets |
| K1500CC | O-ring set | 40.64 x 5.33; 26.57 x 3.53 | Silicon | 5 sets |
| K1500CD | O-ring | 40.64 x 5.33 | Kalrez | 1 |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 |
| O-rings /STW | | | | |
| K1541ZK | O-ring set | 40.87 x 3.53; 26.65 x 2.62; 3" seal-clamp | EPDM | 2 sets |
| O-rings /S2W | | | | |
| K1541ZH | O-ring set | 40.87 x 3.53; 26.65 x 2.62; 2" seal-clamp | EPDM | 2 sets |
| K1500DJ | O-ring set | 40.87 x 3.53; 26.65 x 2.62; 2" seal-clamp | Viton | 2 sets |
| K1500DK | O-ring set | 40.87 x 3.53; 26.65 x 2.62; 2" seal-clamp | Silicon | 2 sets |
| O-rings /TFD, /TFN | | | | |
| K1500AH | O-ring | 29.74 x 3.53 | Kalrez | 1 |
| O-rings /SFT | | | | |
| K1500CM | O-ring set | 18.72 x 2.62; 60 x 3 | EPDM | 5 sets |
| O-rings /STC1 | | | | |
| K1500CQ | O-ring | 18.72 x 2.62 | EPDM | 5 |
| K1500CP | O-ring | 18.72 x 2.62 | Viton | 5 |
| K1500CR | O-ring | 18.72 x 2.62 | Silicon | 5 |
| O-rings /STC2 | | | | |
| K1500CT | O-ring set | 18.72 x 2.72; 2" seal-clamp | EPDM | 5 sets |
| K1500CS | O-ring set | 18.72 x 2.72; 2" seal-clamp | Viton | 5 sets |
| K1500CU | O-ring set | 18.72 x 2.72; 2" seal-clamp | Silicon | 5 sets |

8 EU DECLARATION OF CONFORMITY

YOKOGAWA ♦

EU DECLARATION OF CONFORMITY

We: **Yokogawa Process Analyzers Europe B.V.**
Euroweg 2
3825 HD Amersfoort
The Netherlands

herewith declare under our sole responsibility that the products, model: **ISC40G** and **ISC40S**

further specified with model suffix- and option codes: **As listed in Annex-1 in this document**

are manufactured in accordance with the requirements for CE-marking of products as stated in EC Decision:

768/2008/EC on a common framework for the marketing of products

by applying the following standards:

EN-ISO 9001: 2008 Quality management systems - Requirements

Model ISC40G and ISC40S are:

- In compliance with the essential requirements of the specific product legislation:

- **Pressure Equipment** **Directive 97/23/EC (PED)**

As amended by Regulation (EC) no. 1882/2003, by applying:

Article 3.3: Sound Engineering Practice

- **RoHS** **Directive 2011/65/EU**

by applying:

Category 9: Industrial monitoring and control instruments

- Produced according to appropriate quality control procedures.

Model ISC40S is:

- In compliance with the essential requirements of the specific product legislation:

- **Explosive atmospheres** **Directive 94/9/EC (ATEX)**

As amended by Regulation (EC) no. 1882/2003, by applying the following standards:

EN 60079-0: 2009 Explosive atmospheres – Part 0: Equipment – General requirements

EN 60079-11: 2007 Explosive atmospheres – Part 11: Equipment protection by intrinsic safety "i"

EN 60079-26: 2007 Explosive atmospheres – Part 26: Equipment with equipment protection level (EPL) Ga

The provisions fulfilled are: **Ex II 1 G Ex ia IIC T4...T6 Ga**

Number of the EC-type Examination Certificate: **DEKRA 11 ATEX 0063 X**

Name of the notified body: DEKRA Certification B.V.


Identification number of the notified body: 0344

Address of the notified body: Meander 1051, 6825 MJ Arnhem, The Netherlands

The CE-mark has been affixed on the product in 2000 for the first time.

If applicable, the product is checked against the latest official released revision of the standards mentioned above; differences do not affect the certified product identified on this declaration.

Amersfoort, July 01, 2014


H. Leijten
General Manager
Yokogawa Process Analyzers Europe B.V.

9 ISC40FS – FLOW FITTING SUBASSEMBLY

9.1 General Specifications

9.1.1 Materials

Wetted parts

| | |
|--------------------|------------------------|
| Model ISC40FS-FCSA | : PVDF (Kynar); Viton |
| Model ISC40FS-PCSA | : Polypropylene; Viton |
| Model ISC40FS-SCSA | : AISI 316 SS; Viton |
| Model ISC40FS-SCWN | : AISI 316 SS; Viton |

Non-wetted parts

| | |
|-----|---------------|
| Nut | : AISI 304 SS |
|-----|---------------|

9.1.2 Operating range

Temperature

| | |
|--------------------|----------------------|
| Model ISC40FS-FCSA | : Max. 130°C (266°F) |
| Model ISC40FS-PCSA | : Max. 100°C (212°F) |
| Model ISC40FS-SCSA | : Max. 150°C (302°F) |
| Model ISC40FS-SCWN | : Max. 150°C (302°F) |

Pressure

| | |
|--------------------|--|
| Model ISC40FS-FCSA | : Max. 10 bar (150 PSI) at 20°C (68°F) Max. 1 bar (15 PSI) at 130°C (266°F) |
| Model ISC40FS-PCSA | : Max. 6 bar (90 PSI) at 20°C (68°F) Max. 1 bar (15 PSI) at 100°C (212°F) |
| Model ISC40FS-SCSA | : Max. 10 bar (150 PSI) at operating temperature |
| Model ISC40FS-SCWN | : Max. 10 bar (150 PSI) at operating temperature |

9.1.3 Shipping details

| | |
|-----------------------|---|
| Package size (LxWxH) | : 215 x 150 x 55 mm (8.46 x 5.90 x 2.17 inch) |
| Package weight (max.) | : 0.9 kg (2.0 lbs) |



9.1.4 Process connections

2" screw-in coupling or weld-in coupling

Note: The ISC40 sensor type GG and TG are supplied with a Viton gasket. This gasket may be used with the older series of ISC40FS fittings. It should be discarded when the sensor is mounted in combination with the ISC40FS type FCSA and PCSA.

9.2 Installation of ISC40 sensor in ISC40FS

The key difference between a sensor adapter and a subassembly is, that with subassembly installation the sensor can be removed from the process installation without removing the subassembly first. This allows easier access to the sensor for maintenance activities. Generally, the subassembly consists of three parts of which one part is fitted permanently to the process installation (welded or threaded); the second part is fitted to the sensor and the third part holds the earlier parts together. In addition to these parts there are elastomeric seals were appropriate. Standard O-ring material is Viton, other O-ring materials are available as sparepart (see Figs 15 and 16).

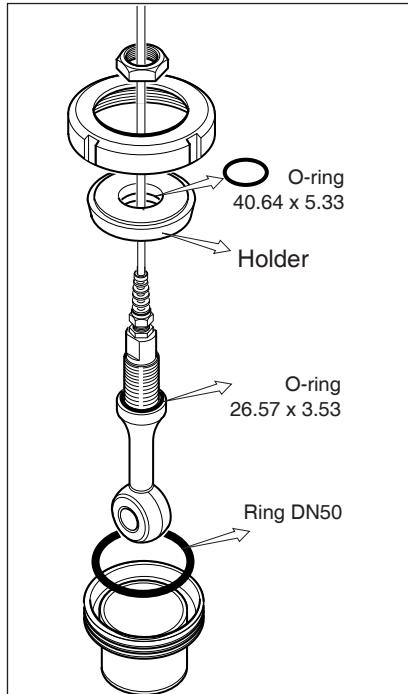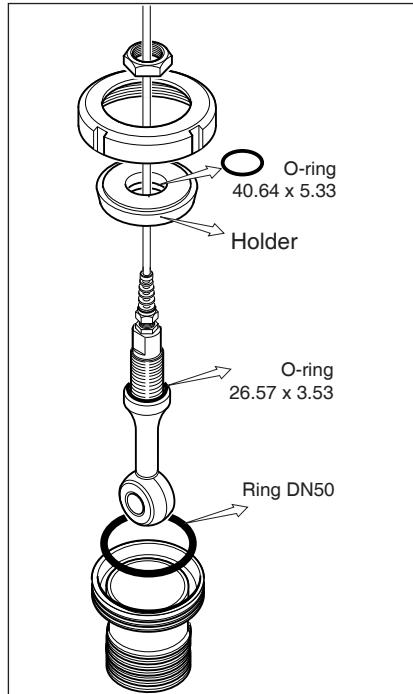

9.3 Dimensions ISC40FS

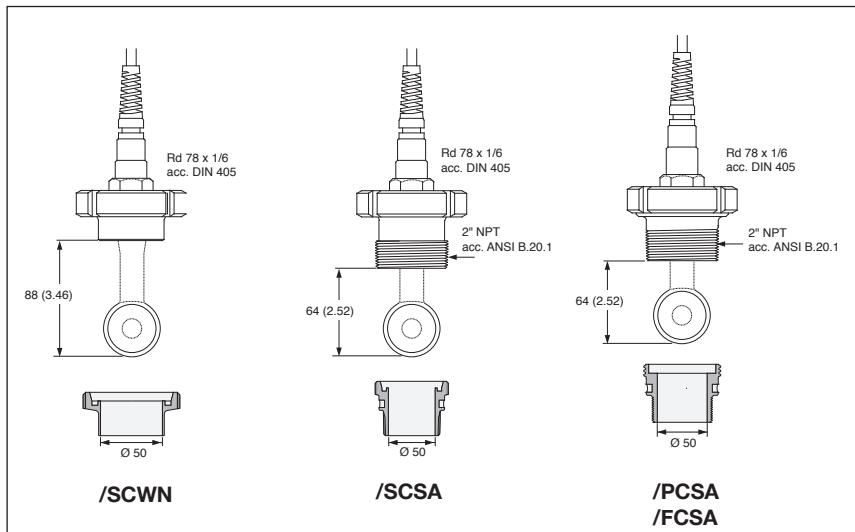


Fig 17: Dimensions ISC40FS with sensor installed (dimensions in mm (inches))

9.4 Modelcode ISC40FS

| Model | Suffix | Option | Description |
|----------------------|----------------|--------|---|
| ISC40FS | | | Flow fitting subassembly |
| Material | -F -P -S | | PVDF Polypropylene Stainless Steel |
| Process connection | -CS -CW | | Dairy Coupling screw-in* Dairy Coupling welded* |
| Thread type NPT or R | -A -N | | NPT No thread (for weld-in couplings) |
| Options | /M | | Material certificate 3.1. EN 10024 (for wetted metal parts only) |

* Note: according to Din 11851

9.5 Spareparts ISC40FS

| Parts ISC40FS subassembly | | | | |
|---------------------------|------------------|------------|---------------|--------|
| Part no. | Description | Dimensions | Material | O-ring |
| K1541KD | Holder + O-rings | 2" | PVDF | Viton |
| K1541KL | Holder + O-rings | 2" | Polypropylene | Viton |
| K1541KA | Holder + O-rings | 2" | AISI 316 SS | Viton |

Note: Other O-ring materials are available as sparepart

| O-rings ISC40FS subassembly | | | | | |
|---|-------------|--|----------|----------|--|
| Part no. | Description | Dimensions | Material | Quantity | |
| O-rings -FCSA, -PCSA, -FCWN, -PCWN | | | | | |
| K1500DF | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | EPDM | 5 sets | |
| K1500DE | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | Viton | 5 sets | |
| K1500DG | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | Silicon | 5 sets | |
| K1500CD | O-ring | 40.64 x 5.33 | Kalrez | 1 | |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 | |
| O-rings -SCSA, -SCWN | | | | | |
| K1500DB | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | EPDM | 5 sets | |
| K1500DA | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | Viton | 5 sets | |
| K1500DC | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | Silicon | 5 sets | |
| K1500CD | O-ring | 40.64 x 5.33 | Kalrez | 1 | |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 | |
| K1500DD | O-ring | 53.34 x 5.33 | Kalrez | 1 | |

Note: O-ring 53.34 x 5.33 (K1500DD) is used as a Kalrez replacement for the Ring DN50.

10 ISC40FF – FLOW FITTING

10.1 General Specifications

10.1.1 Materials

Wetted parts

| | |
|-------------------------|------------------------------|
| Model ISC40FF-S | : AISI 316 SS; Viton |
| Model ISC40FF-P | : Polypropylene; Viton |
| Model ISC40FF-F | : PVDF (Kynar); Viton |
| Non-wetted parts | : AISI 304 SS or AISI 316 SS |

10.1.2 Operating range

Temperature

| | |
|-----------------|----------------------|
| Model ISC40FF-S | : Max. 150°C (302°F) |
| Model ISC40FF-P | : Max. 100°C (212°F) |
| Model ISC40FF-F | : Max. 130°C (266°F) |

Pressure

| | |
|-----------------|--|
| Model ISC40FF-S | : Max. 10 bar (150 PSI) at operating temperature |
| Model ISC40FF-P | : Max. 6 bar (90 PSI) at 20°C (68°F) Max. 1 bar (15 PSI) at 100°C (212°F) |
| Model ISC40FF-F | : Max. 10 bar (150 PSI) at 20°C (68°F) Max. 1 bar (15 PSI) at 130°C (266°F) |

10.1.3 Shipping details

| | |
|----------------------|--|
| Package size (LxWxH) | : 250 x 150 x 100 mm (9.84 x 5.90 x 3.94 inch) |
| Package weight (max) | : 1.5 kg (3.3 lbs) |

10.1.4 Process connections

1/2" NPT in flow fitting, connected with optional flange adapters to the actual installation.

Note: The ISC40 sensor type -GG and -TG are supplied with a Viton gasket. This gasket may be used with the older series of ISC40FF fittings. It should be discarded when the sensor is mounted in combination with the ISC40FF type -PA and -FA.

10.2 Installation of ISC40 sensor in ISC40FF

Installation of the flow fittings involves two steps (see Fig 18):

- Installation of the sensor

The sensor has to be mounted in the flow fitting. It is important that the position of the sensor in the fitting allows easy flow through the hole of the sensor donut. Generally good flow is assured if the flats of the sensor are oriented perpendicular to the outlet piping. It is also important that the sample piping is oriented in such a way that the direction of the flow is upwards to assure complete filling of the flow chamber

- Installation of the fitting on wall, railing or stanchion

For this purpose the flow fitting has an optional pipe/wall mounting kit /MS or /MP (see Fig 19 for details). This kit consists of a clamp ring with bolts and nuts which clamps around the flow chamber. Therefore the flow chamber can be turned in the mounting assembly allowing more flexibility in installation. The mounting plate can be mounted on a wall or panel with 2-4 anchor bolts with a diameter of 10 mm (3/8") max. For those installations where pipe mounting is requested (2" nominal pipe), either horizontal or vertical, a saddle and U-bolt have to be used.

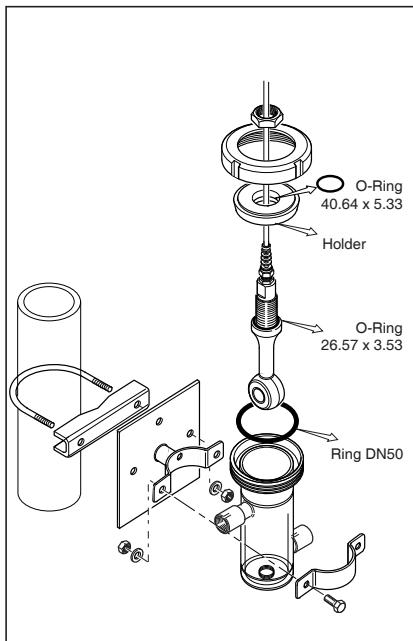


Fig 18: Installation of ISC40 sensor in flow fitting

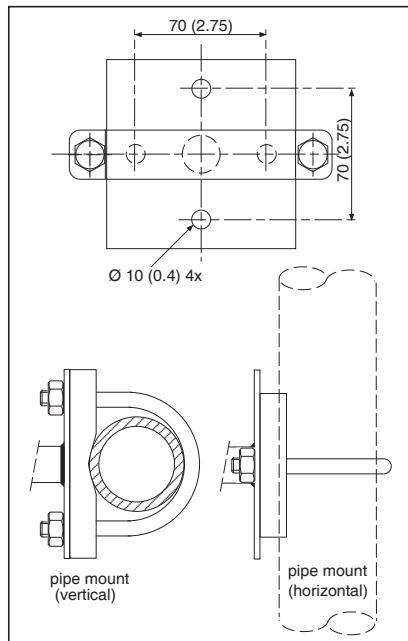


Fig 19: Pipe/wall mounting kit

Note: The ISC40 sensor type -TG does not fit in the model ISC40FF-S.

10.3 Dimensions ISC40FF

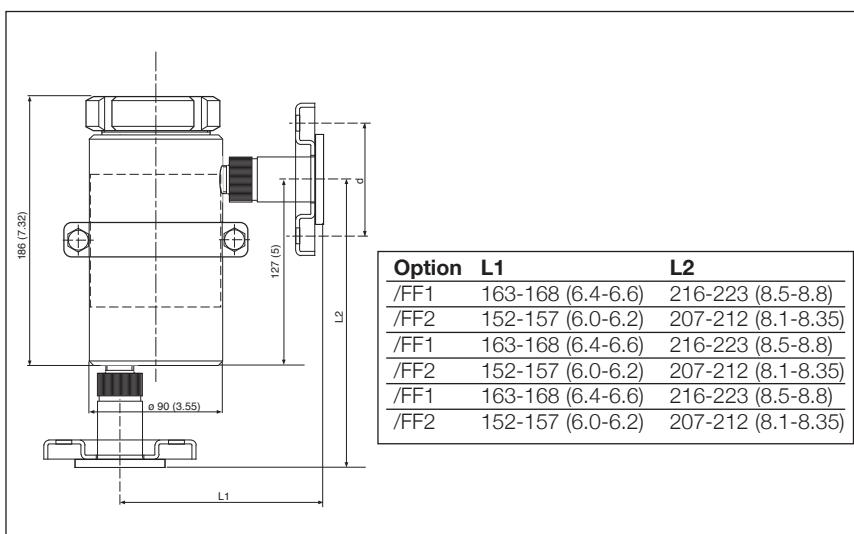


Fig 20: Flow fitting ISC40FF-P, ISC40FF-F

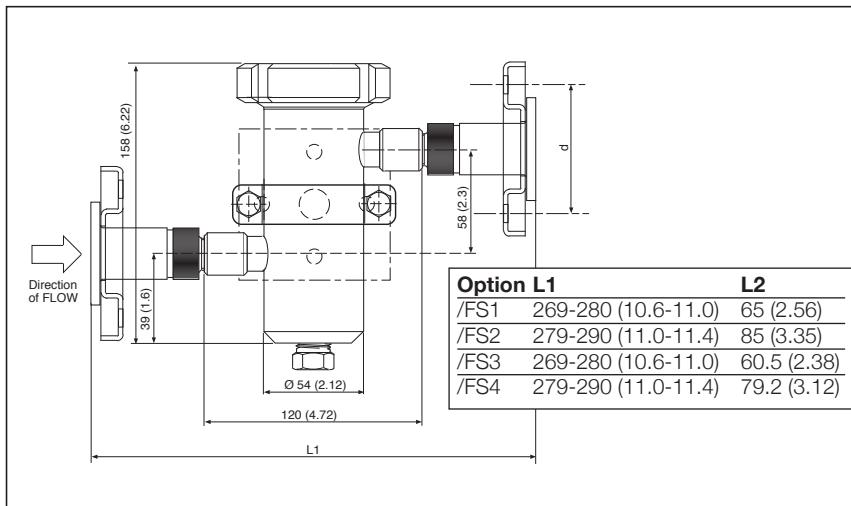


Fig 21: Flow fitting ISC40FF-S

10.4 Modelcode ISC40FF

| Model | Suffix | Option | Description |
|-------------------------|--|--------|--|
| ISC40FF | | | flow fitting |
| Material | -S -P -F | | AISI 316 stainless steel Polypropylene (PP) PVDF (KYNAR®) |
| Process connection | -A | | NPT |
| 1/2"NPT Flange adapters | /FF1 /FF2 /FF3 /FF4 /FP1 /FP2 /FP3 /FP4 /FS1 /FS2 /FS3 /FS4 | | PVDF, DN15 PN10 PVDF, DN25 PN10 PVDF, ANSI 1/2"-150lbs PVDF, ANSI 1"-150lbs PP, DN15 PN10 PP, DN25 PN10 PP, ANSI 1/2"-150lbs PP, ANSI 1"-150lbs AISI 316 SS, DN15 PN10 AISI 316 SS, DN25 PN10 AISI 316 SS, ANSI 1/2"- 150lbs AISI 316 SS, ANSI 1"- 150lbs |
| Mounting set | /MS /MP | | Wall/pipe for SS flow fitting Wall/pipe for PP or PVDF flow fitting |
| Material certificate | /M | | 3.1. according EN 10024 (for wetted metal parts only) |

10.5 Spareparts ISC40FF

| Options ISC40FF Flow fitting, flange adapters | | | | |
|--|-------------|--------------------|-------------|-----------|
| Part no. | Description | Process connection | Material | O-ring(s) |
| K1521AL | /FF1 | DN15 PN10 | PVDF | Viton |
| K1521AP | /FF2 | DN25 PN10 | PVDF | Viton |
| K1521AE | /FF3 | ANSI ½" – 150 lbs | PVDF | Viton |
| K1521AH | /FF4 | ANSI 1" – 150 lbs | PVDF | Viton |
| K1521AM | /FP1 | DN15 PN10 | PP | Viton |
| K1521AQ | /FP2 | DN25 PN10 | PP | Viton |
| K1521AF | /FP3 | ANSI ½" – 150 lbs | PP | Viton |
| K1521AJ | /FP4 | ANSI 1" – 150 lbs | PP | Viton |
| K1521AK | /FS1 | DN15 PN10 | AISI 316 SS | Viton |
| K1521AN | /FS2 | DN25 PN10 | AISI 316 SS | Viton |
| K1521AD | /FS3 | ANSI ½" – 150 lbs | AISI 316 SS | Viton |
| K1521AG | /FS4 | ANSI 1" – 150 lbs | AISI 316 SS | Viton |

Note: Other O-ring materials are available as sparepart

| Parts ISC40FF Flow fitting | | | | |
|-----------------------------------|------------------|------------|---------------|--------|
| Part no. | Description | Dimensions | Material | O-ring |
| K1541KD | Holder + O-rings | 2" | PVDF | Viton |
| K1541KL | Holder + O-rings | 2" | Polypropylene | Viton |
| K1541KA | Holder + O-rings | 2" | AISI 316 SS | Viton |

Note: Other O-ring materials are available as sparepart

| O-rings ISC40FF Flow fitting | | | | |
|-------------------------------------|-------------|--|----------|----------|
| Part no. | Description | Dimensions | Material | Quantity |
| O-rings -SA | | | | |
| K1500DB | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | EPDM | 5 sets |
| K1500DA | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | Viton | 5 sets |
| K1500DC | O-ring set | 40.64 x 5.33; 26.57 x 3.53; Ring DN50 | Silicon | 5 sets |
| K1500CD | O-ring | 40.64 x 5.33 | Kalrez | 1 |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 |
| K1500DD | O-ring | 53.34 x 5.33 | Kalrez | 1 |
| O-rings -PA, -FA | | | | |
| K1500DF | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | EPDM | 5 sets |
| K1500DE | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | Viton | 5 sets |
| K1500DG | O-ring set | 40.64 x 5.33; 26.57 x 3.53; 56.52 x 5.33 | Silicon | 5 sets |
| K1500CD | O-ring | 40.64 x 5.33 | Kalrez | 1 |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 |

Note: O-ring 53.34 x 5.33 (K1500DD) is used as a Kalrez replacement for the Ring DN50.

11 ISC40FD – IMMERSION FITTING

11.1 General Specifications

11.1.1 Materials

Wetted parts without options

| | |
|-------------------------|----------------------|
| Model ISC40FD-S | : AISI 316 SS, Viton |
| Model ISC40FD-V | : C-PVC, Viton |
| Flange ISC40FD-S-**-SF* | : AISI 316 SS |

Non-wetted parts

| | |
|--------------|-----------|
| Tube pigtail | : plastic |
|--------------|-----------|

11.1.2 Operating range

Temperature

| | |
|-----------------|----------------------|
| Model ISC40FD-S | : Max. 150°C (302°F) |
| Model ISC40FD-V | : Max. 80°C (176°F) |

Pressure

| | |
|-----------------|---|
| Model ISC40FD-S | : Max. 10 bar (150 PSI) at operating temperature |
| Model ISC40FD-V | : Max. 2 bar (30 PSI) at 20°C (68°F) Max. 1 bar (15 PSI) at 80°C (176°F) |

11.1.3 Process connections

Flange AISI 316 SS 2" or AISI 316 SS DN50, for the type -V an adjustable optional flange is available with ANSI 2" 150 lbs and DN50 PN10 hole pattern.

Note: The ISC40 sensor type -GG and -TG are supplied with a Viton gasket. This gasket may be used with the older series of ISC40FD fittings. It should be discarded when the sensor is mounted in combination with the ISC40FD type -S and -V.

11.2 Installation of ISC40 sensor in ISC40FD

Installation of the immersion fittings involves two steps:

- Installation of the sensor
The sensor has to be mounted in the immersion fitting (see Fig 22).
- Installation in the application
 - o On a railing or stanchion
For this purpose the immersion fitting has an optional rail mounting kit /MS1. This kit consists of a piece of guide pipe and two pipe clamps. The guide pipe is mounted horizontally to the stanchion using one pipe clamp. The second pipe clamp connects the guide pipe to the immersion fitting. The distance between the pipe clamps determines the distance between the stanchion and immersion fitting (see Fig 23).
 - o With flange
For this purpose a stainless steel immersion fitting can be ordered as type -SFD (DN50) or type -SFA (2"). The PVC immersion fitting has an optional depth adjustable mounting flange /FA (with DN50 and ANSI 2" 150 lbs hole pattern) which is illustrated in Fig 24. You must assure that the mating flange has the same hole pattern as the supplied flange.

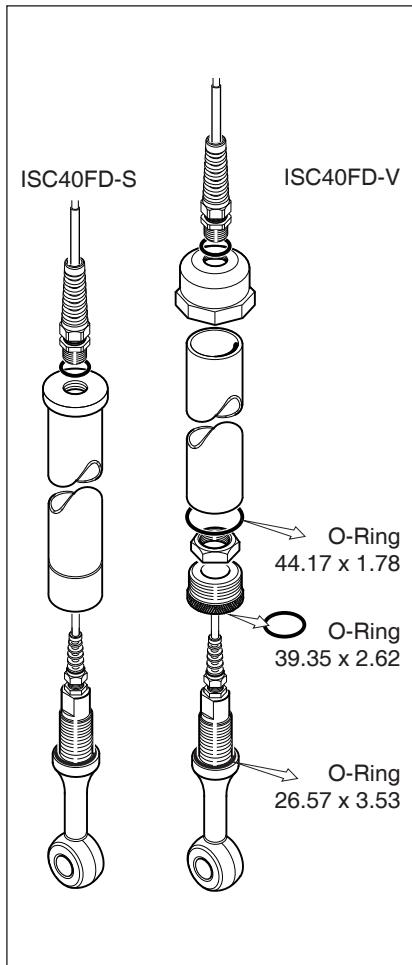


Fig 22: Installation of ISC40 sensor in immersion fitting.

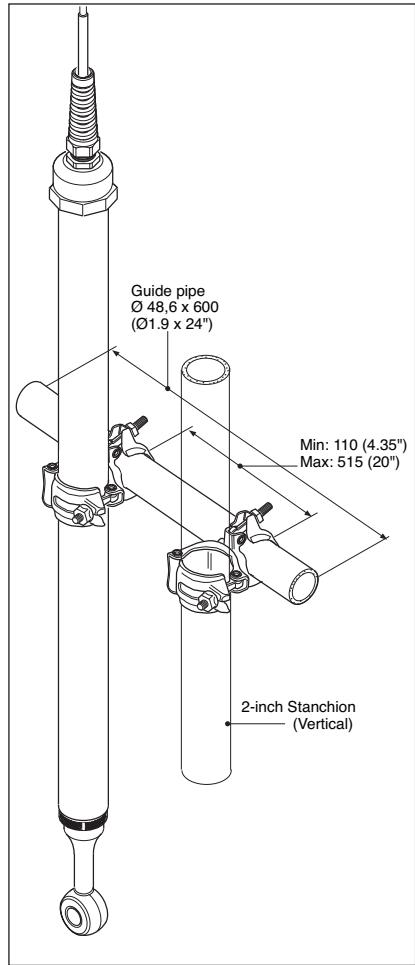


Fig 23: Installation on stanchion with /MS1

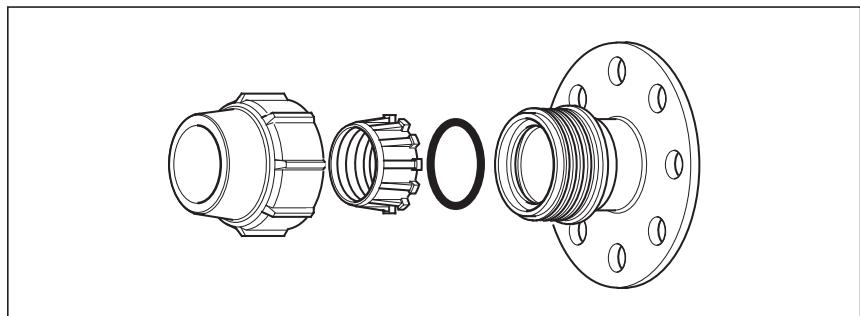


Fig 24: Option /FA

Alternative ways of mounting the immersion fitting are:

- Guide pipe

To facilitate this type of mounting the immersion fitting has a larger diameter at the top.

The user supplied guide pipe (internal diameter > 52 mm) is fitted to the wall or mounting rail. The immersion fitting slides into this guide pipe and therefore the sensor can be easily removed for inspection.

- Platform mounting

Sometimes there is a walking platform that can be used to mount the immersion fitting.

The top of the immersion fitting has a larger diameter than the shaft. The only thing to do is to drill a precise hole in the platform to slide the fitting through.

11.3 Dimensions ISC40FD

Dimensions in mm (inches)

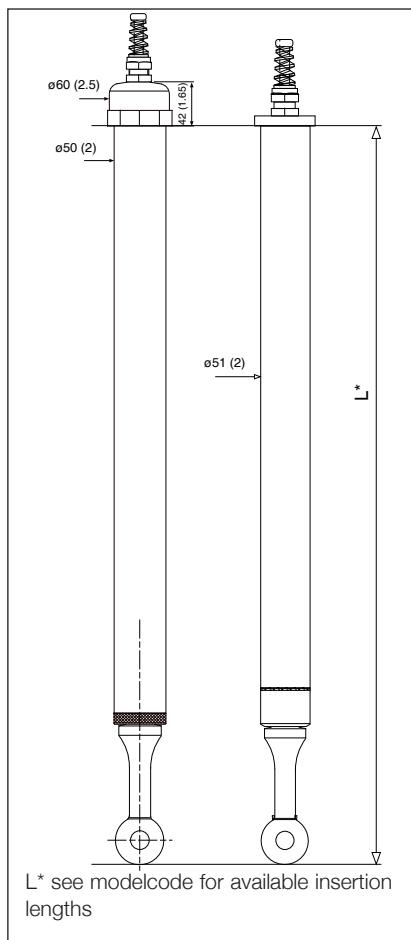


Fig 25: Immersion fitting ISC40FD

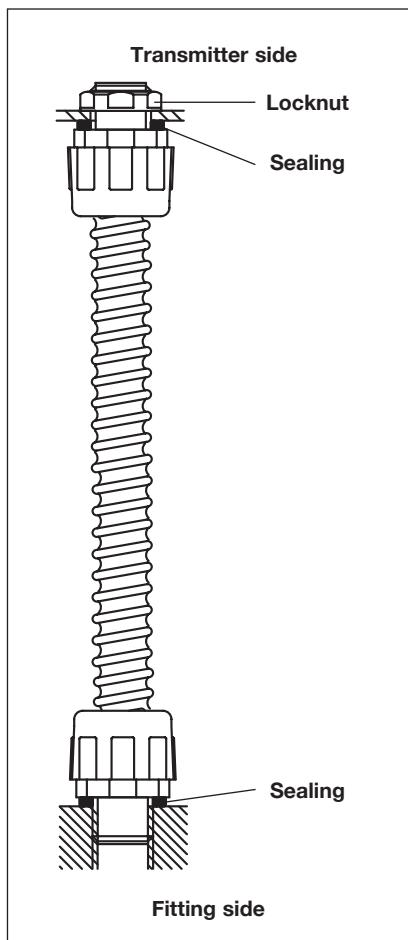


Fig 26: Protection hose, option /PH5, /PH10

11.4 Modelcode ISC40FD

| Model code | Suffix code | Option code | Description |
|----------------------|----------------------|----------------------------------|--|
| ISC40FD | | | Immersion fitting |
| Material | -S -V | | AISI 316 Stainless steel PVC-C |
| Insertion length | - □ □ | | Between 05 to 20 Example: 05 = 0.5 m / 20 = 2.0 m |
| Flange | -NFL -SFA -SFD | | No flange AISI316 SS 2" AISI316 SS DN50 |
| Options | | /MS1 /FA /PH5 /PH10 | Pipe mounting set (Carbon steel) Adjustable flange with DIN DN50-PN10 and ANSI 2" 150 lbs hole pattern (only for PVC) Protection hose for 5 m cable Protection hose for 10 m cable |
| Material certificate | | /M | 3.1. according EN 10204 (for wetted metal parts only) |

Note: option /FA only for ISC40FD-V; option /M only for ISC4FD-S

11.5 Spareparts ISC40FD

| Options ISC40FD Flow fitting | | | | |
|-------------------------------------|-------------|------------------------|--------------|--|
| Part no. | Description | Process connection | Material | |
| K1541ZY | /MS1 | | Carbon steel | |
| K1520EV | /FA | DN50 PN10; ANSI 2" lbs | PP | |
| K1500CJ | /PH5 | | PVC, PA6.6 | |
| K1500CK | /PH10 | | PVC, PA 6.6 | |

| O-rings ISC40FD Immersion fitting | | | | |
|--|-------------|--|----------|----------|
| Part no. | Description | Dimensions | Material | Quantity |
| O-rings -S | | | | |
| K1500CE | O-ring set | 39.35 x 2.62; 26.57 x 3.53 | EPDM | 5 sets |
| K1500CF | O-ring set | 39.35 x 2.62; 26.57 x 3.53 | Viton | 5 sets |
| K1500CG | O-ring set | 39.35 x 2.62; 26.57 x 3.53 | Silicon | 5 sets |
| K1500CH | O-ring | 26.57 x 3.53 | Kalrez | 1 |
| O-rings -V | | | | |
| K1500CX | O-ring set | 39.35 x 2.62; 26.57 x 3.53; 44.17 x 1.78 | EPDM | 5 sets |
| K1500CW | O-ring set | 39.35 x 2.62; 26.57 x 3.53; 44.17 x 1.78 | Viton | 5 sets |
| K1500CY | O-ring set | 39.35 x 2.62; 26.57 x 3.53; 44.17 x 1.78 | Silicon | 5 sets |

12 Chemical Compatibility Chart

| | | Material | | | | | | |
|---------------------|----------------------|-----------------|-----------------|-----------------|----------|----------|-----------------|-----------|
| | | PVDF (Kynar) | S.S. 316 | VITON | PEEK | PP | PVC | PFA |
| Temp. % Conc. | 20 60 100 | 20 60 100 | 20 60 100 | 20 60 100 | 20 60 | 20 60 | 20 60 100 | |
| Inorganic acid | Sulfuric acid | 10 O O O | XXX | O O O | O O | O X | O O O | |
| | | 50 O O O | XXX | O O O | O O | O O | O O O O O | |
| | | 95 O X - | XXX | O O O | - - - | X - | XX | O O O |
| | fuming | - - - | - - - | O O O | - - - | - - - | - - - | O O O |
| | Hydrochloric acid | 10 O O O | - - - | O O O | O O X | O O | O X | O O O |
| | | sat. O O O | - - - | | O O X | O O | O O | O O O |
| | Nitric acid | 25 O O X | XXX | O O X | O O O | O O | O X | O O O |
| | | 50 O O X | XXX | - - - | XXX | X - | O X | O O O |
| | | 95 O X - | O O O | - - - | - - - | - - - | - - - | O O O |
| | | fuming | - - - | O O O | - - - | - - - | - - - | O O O |
| | Phosphoric acid | 25 O O O | - - - | O O O | O O O | O O | O X | O O O |
| | | 50 O O O | XXX | O O O | O O O | O O | O O | O O O |
| | | 95 O O O | O O O | XX - | O O O | O O | O O | O O O |
| | Hydrofluoric acid | 40 O O O | - - - | O O O | - - - | O O | O X | O O O |
| | | 75 O O O | - - - | O O O | - - - | O O | XX | O O O |
| | | | | | | | | |
| Organic acid | Acetic acid | 10 O O O | O O X | - - - | O O O | O O | O X | O O O |
| | | glacial O X - | O O X | - - - | O O X | O X | XX | O O O |
| | Formic acid | 80 O O O | XXX | - - - | XXX | O O | O - | O O X |
| | Citric acid | 50 O O O | O O O | O O O | O O O | O O | O O | O O O |
| Alkali | Calcium hydroxide | sat. O O O | O O O | O O O | O O O | O O | O O | O O O |
| | Potassium hydroxide | 50 O O X | O O O | O O O | O O O | O O | O O | O O O |
| | Sodium hydroxide | 40 O O X | O O O | XXX | O O O | O O | O X | O O O |
| | Ammonia in water | 30 O O O | O O O | XXX | O O O | O O | O X | O O O |
| salt | Ammonium chloride | sat. O O O | XXX | O O O | O O O | O O | O O | O O O |
| | Zinc chloride | 50 O O O | XXX | O O O | O O O | O O | O O | O O O |
| | Iron (III) chloride | 50 O O O | - - - | O O O | O O O | O O | O O | O O O |
| | | | | | | | | |
| salt | Sodium sulfite | sat. O O O | O O O | - - - | O O O | O O | O O | O O O |
| | Sodium carbonate | sat. O O O | O O O | O O O | O O O | O O | O O | O O O |
| | | | | | | | | |
| | Potassium chloride | sat. O O O | XXX | O O O | O O O | O O | O O | O O O |
| salt | Sodium sulfate | sat. O O O | O O O | O O O | O O O | O O | O O | O O O |
| | Calcium chloride | sat. O O O | XXX | O O O | O O O | O O | O O | O O O |
| | Sodium chloride | sat. O O O | XXX | O O O | O O O | O O | O O | O O O |
| | Sodium nitrate | 50 O O O | XXX | O O O | O O O | O O | O O | O O O |
| salt | Aluminium chloride | sat. O O O | - - - | O O O | O O O | O O | O O | O O O |
| | | | | | | | | |
| | Hydrogen peroxide | 30 O O O | O O O | O O O | O O O | O O | O O | O O O |
| | Sodium hypochlorite | 50 O O O | XXX | O O X | O O O | XX | XX | O O O |
| agent | Potassium dichromate | sat. O O O | O O O | O O O | O O O | O O | O O | O O O |
| | Chlorinated lime | | O X - | XXX | | XXX | - - | O O O O O |
| | | | | | | | | |
| | Ethanol | 80 O O X | O O O | X - - | O O O | O O | O X | O O O |
| solvent | Cyclohexane | | O O X | O O O | O O O | O O | O O | O O O |
| | Toluene | | O O O | O O O | - - - | O O O | X - | - - O O O |
| | Trichloroethane | | XXX | O O X | XXX | O O O | - - | - - O O O |
| | Water | | O O O | O O O | O O O | O O | O O | O O O |

O = can be used, X = shortens useful life, - = cannot be used

Note: Information in this list is based on our general experience and literature data and given in good faith. However Yokogawa is unable to accept responsibility for claims related to this information.

YOKOGAWA ELECTRIC CORPORATION
World Headquarters
9-32, Nakacho 2-chome, Musashino-shi
Tokyo 180-8750
Japan
www.yokogawa.com

YOKOGAWA CORPORATION OF AMERICA
2 Dart Road
Newnan GA 30265
USA
www.yokogawa.com/us

YOKOGAWA EUROPE BV
Europeweg 2
3825 HD AMERSFOORT
The Netherlands
www.yokogawa.com/eu

YOKOGAWA ELECTRIC ASIA Pte. LTD.
5 Bedok South Road
Singapore 469270
Singapore
www.yokogawa.com/sg

YOKOGAWA CHINA CO. LTD.
3F Tower D Cartelo Crocodile Building
No.568 West Tianshan Road Changning District
Shanghai, China
www.yokogawa.com/cn

YOKOGAWA MIDDLE EAST B.S.C.(c)
P.O. Box 10070, Manama
Building 57/, Road 2516, Busaitteen 225
Muharraq, Bahrain
www.yokogawa.com/bh

Yokogawa has an extensive sales and distribution network.
Please refer to the European website (www.yokogawa.com/eu) to contact your nearest representative.



YOKOGAWA ♦